



# TEST REPORT: GSM90A48-P1M

## 90W AC-DC High Reliability Medical Adaptor

### ■ DESIGN VERIFY TEST

- Output Function Test
- Input Function Test
- Protection Function Test
- Component Stress Test

### ■ SAFETY & E.M.C. TEST

- Safety Test
- E.M.C. Test

### ■ RELIABILITY TEST

- ENVIRONMENT TEST


DESIGN VERIFY TEST  
OUTPUT FUNCTION

| NO | TEST ITEM  | SPECIFICATION                      | TEST CONDITION   | RESULT                           |
|----|--|------------------------------------|--|----------------------------------|
| 1  | OUTPUT VOLTAGE RANGE   | CH1: 46.80V ~ 49.20V               | I/P : 230VAC<br>O/P: MIN LOAD<br>TA : 25°C   | CH1: 47.57V ~ 47.57V             |
| 2  | OUTPUT VOLTAGE TOLERANCE (Max)   | V1 : 2.5% ~ -2.5%                  | I/P : 100VAC / 264VAC<br>O/P: FULL / MINLOAD<br>TA= 25°C                             | V1: -0.92% ~ -1.56%              |
| 3  | LINE REGULATION (MAX.)   | V1 : 1.0% ~ -1.0%                  | I/P : 100VAC / 264VAC<br>O/P: FULL LOAD<br>TA : 25°C                                 | V1: 0.08% ~ -0.02%               |
| 4  | LOAD REGULATION (MAX.)   | V1 : 2.5% ~ -2.5%                  | I/P : 230VAC<br>O/P: MIN LOAD ~ FULL LOAD<br>TA : 25°C                               | V1: 0.32% ~ -0.32%               |
| 5  | OVER/UNDERSHOOT TEST   | < ±5%                              | I/P : 230VAC<br>O/P: FULL LOAD<br>TA : 25°C  | TEST< 1.7 %                      |
|    | RIPPLE & NOISE(Max)  | V1 : 200 mVp-p                     | I/P : 230VAC<br>O/P: FULL LOAD<br>TA : 25°C  | V1 : 27.6 mVp-p                  |
| 6  | <p>high frequency :</p>  |                                    | <p>low frequency :</p>   |                                  |
| 7  | SET UP TIME (MAX.)   | 230VAC : 1000ms<br>115VAC : 1000ms | I/P : 230VAC<br>I/P : 115VAC<br>O/P: FULL LOAD<br>TA : 25°C                          | 230VAC : 428ms<br>115VAC : 456ms |
|    | <p>INPUT=230VAC/50HZ @ FULL LOAD<br/>CH1 : Output Voltage CH2 : AC Input Voltage</p> |                                    | <p>INPUT=115VAC/60HZ @ FULL LOAD<br/>CH1 : Output Voltage CH2 : AC Input Voltage</p> |                                  |

|    |  |                                |   |                                      |
|----|--|--------------------------------|---|--------------------------------------|
| 8  | RISE TIME (MAX.)   | 230VAC : 50ms<br>115VAC : 50ms | I/P : 230VAC<br>I/P : 115VAC<br>O/P: FULL LOAD<br>TA: 25°C  | 230VAC : 24.4ms<br>115VAC : 23.7ms   |
|    | INPUT=230VAC/50HZ @ FULL LOAD<br>CH1 : Output Voltage                        |                                | INPUT=115VAC/60HZ @ FULL LOAD<br>CH1 : Output Voltage   |                                      |
|    |  |                                |   |                                      |
| 9  | HOLD UP TIME (TYP.)  | 230VAC : 20ms<br>115VAC : 20ms | I/P : 230VAC<br>I/P : 115VAC<br>O/P: FULL LOAD<br>TA: 25°C  | 230VAC : 37.2ms<br>115VAC : 26.4ms   |
|    | INPUT=230VAC/50HZ @ FULL LOAD<br>CH1 : Output Voltage CH2 : AC Input Voltage |                                | INPUT=115VAC/60HZ @ FULL LOAD<br>CH1 : Output Voltage CH2 : AC Input Voltage                          |                                      |
|    |  |                                |   |                                      |
| 10 | DYNAMIC LOAD   | V1 : 4800 mVp-p                | I/P : 230VAC<br>O/P:<br>(1)Full/Min load 50% duty/120HZ<br>(2)Full/Min load 50% duty/1KHZ<br>TA: 25°C | V1: (1). 968mv (2). 832mv unit:mVp-p |
|    | FULL /Min LOAD 50%DUTY / 120HZ   |                                | FULL /Min LOAD 50%DUTY / 1KHZ   |                                      |
|    |  |                                |   |                                      |

INPUT FUNCTION TEST

| NO | TEST ITEM                 | SPECIFICATION                      | TEST CONDITION   | RESULT                                    |
|----|---------------------------|------------------------------------|--|---|
| 1  | INPUT VOLTAGE RANGE       | 80VAC ~ 264VAC                     | I/P : TESTING<br>O/P : FULL LOAD<br>Ta : 25°C  | 58.0VAC ~ 264VAC                          |
|    |                           |                                    | I/P :<br>LOW-LINE = 97VAC<br>HIGH-LINE = 300VAC<br>O/P : FULL/MIN LOAD<br>ON:30 Sec ; OFF:30 Sec 10MIN<br>(POWER ON/OFF NO DAMAGE) | TEST : OK                                 |
| 2  | INPUT FREQUENCY RANGE     | 47HZ ~ 63HZ<br>NO DAMAGE           | I/P : 100VAC ~ 264VAC<br>O/P : FULL-MIN LOAD<br>Ta : 25°C  | TEST : OK                                 |
| 3  | INPUT CURRENT (TYP.)      | 0.6 / 230VAC<br>1.3 / 115VAC       | I/P : 230VAC<br>I/P : 115VAC<br>O/P : FULL LOAD<br>TA : 25°C   | I= 0.4404 / 230VAC<br>I= 0.851 / 115VAC   |
| 4  | LEAKAGE CURRENT           | < 0.10mA for earth leakage current | I/P : 264VAC<br>O/P : MIN LOAD<br>TA : 25°C  | L-FG: 0.078 mA<br>N-FG: 0.076 mA          |
|    |                           | < 0.10mA for touch leakage current | I/P : 264VAC<br>O/P : MIN LOAD<br>TA : 25°C  | L-V-: 0.086 mA<br>N-V-: 0.087 mA          |
| 5  | NO LOAD POWER CONSUMPTION | < 0.15W                            | I/P : 230VAC<br>O/P : MIN LOAD<br>TA : 25°C  | < 0.1111 W                                |
| 6  | POWER FACTOR (TYP.)       | 0.91 / 230VAC<br>0.95 / 115VAC     | I/P : 230VAC<br>I/P : 115VAC<br>O/P : FULL LOAD<br>TA : 25°C   | PF= 0.952 / 230VAC<br>PF= 0.9878 / 115VAC |
|    |                           |                                    |  |   |
| 7  | EFFICIENCY (TYP.)         | 91.0%                              | I/P : 230VAC<br>O/P : FULL LOAD<br>TA : 25°C   | 91.363 %                                  |
|    |                           |                                    |  |   |

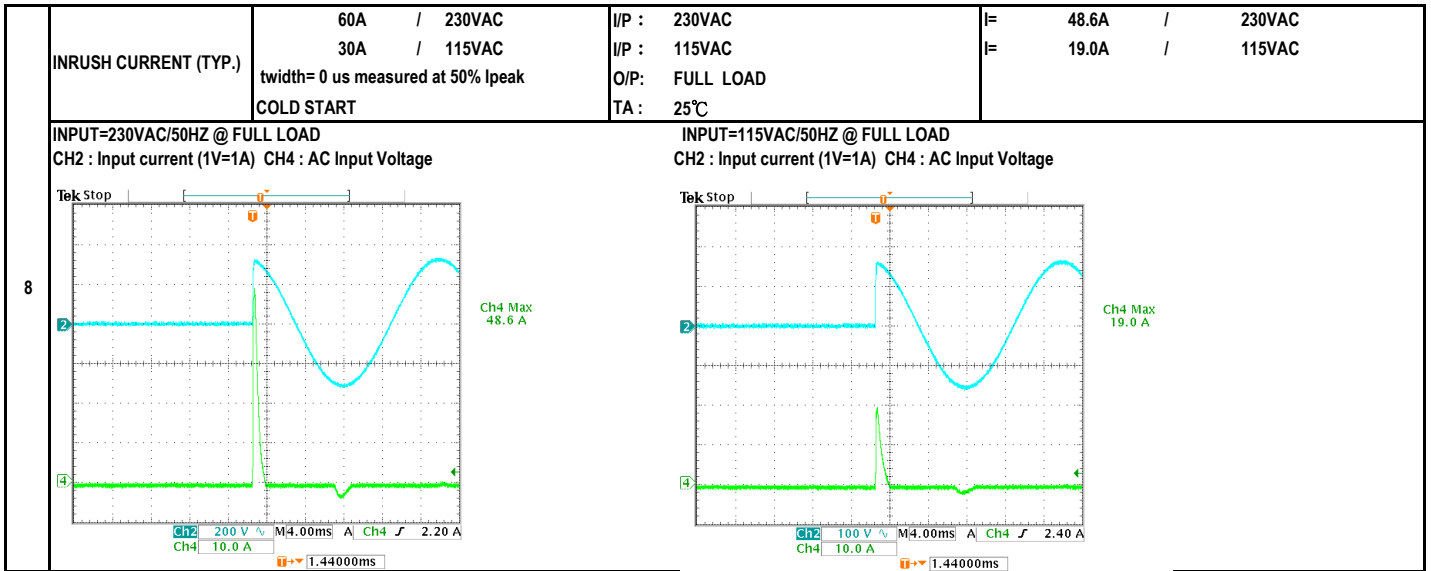

**PROTECTION FUNCTION TEST**

| NO | TEST ITEM                   | SPECIFICATION                          | TEST CONDITION   | RESULT   |
|----|-----------------------------|--|--|--|
| 1  | OVER LOAD PROTECTION        | 110% ~ 150%                            | I/P: 264VAC<br>I/P: 230VAC<br>I/P: 100VAC<br>O/P: TESTING<br>TA : 25°C | 134% 264VAC<br>134% 230VAC<br>130% 100VAC<br>Hiccup Mode                 |
| 2  | OVER VOLTAGE PROTECTION     | 50.40V ~ 64.80V                        | I/P: 264VAC<br>I/P: 230VAC<br>I/P: 80VAC<br>O/P: MIN LOAD<br>TA : 25°C | 58.00V 264VAC<br>58.00V 230VAC<br>58.00V 80VAC<br>Shut down Re- power ON |
| 3  | OVER TEMPERATURE PROTECTION | Shut down Re- power ON                 | I/P: 264VAC<br>I/P: 80VAC<br>O/P: FULL LOAD<br>TA : 25°C               | O.T.P. Active<br>Shut down Re- power ON                                  |
| 4  | SHORT PROTECTION            | SHORT EVERY OUTPUT<br>1 HOUR NO DAMAGE | I/P: 264VAC<br>I/P: 80VAC<br>O/P: FULL LOAD<br>Ta: 25°C                | NO DAMAGE<br>Hiccup Mode   |

**COMPONENT STRESS TEST**

| NO | TEST ITEM            | SPECIFICATION           | TEST CONDITION  | RESULT  |
|----|----------------------|-------------------------|---|---|
| 1  | PWM Power Transistor | Q32 Rated : 700V 11.0A  | I/P : 267VAC<br>VDS :<br>O/P : (1)Full Load Turn on<br>(2) Output Short<br>(3)Full load continue<br>Ta : 25°C             | VIN: 267VAC<br>VDS:<br>(1). 602.00V<br>(2). 506.00V<br>(3). 584.00V |
| 2  | O/P Diode (MOSFET)   | Q101 Rated : 400V 10.0A | I/P : 267VAC<br>VDS :<br>O/P : (1)Full Load Turn on<br>(2) Output Short<br>(3)Full load continue<br>Ta : 25°C             | Q101<br>VDS :<br>(1). 229.00V<br>(2). 249.00V<br>(3). 209.00V       |
| 3  | Input Capacitor      | C5 Rated : 100uf 400V   | I/P : 267VAC<br>O/P : (1)Full Load Turn on /Off<br>(2)Min load Turn on /Off<br>(3)Full Load /Min load Change<br>Ta : 25°C | (1). 405.00V<br>(2). 403.00V<br>(3). 403.00V                        |

|   |                      |  |   |   |
|---|----------------------|--|---|---|
| 4 | Control IC           | U2<br>Rated : 28V (max)<br>-0.3V (min) | I/P : 267VAC<br>O/P : (1)Full Load<br>(2)Output Short<br>(3)O.L.P<br>(4)O.V.P<br>(5)Low Line No Load Vo(min)<br>Ta : 25°C   | U2<br>(1). 18.50V<br>(2). 15.00V<br>(3). 16.90V<br>(4). 21.40V<br>(5). 18.80V |
| 5 | PFC Power Transistor | Q31<br>Rated : 600V 15.8A              | I/P : 267VAC<br>VDS :<br>O/P : (1)Full Load Turn on<br>(2) Output Short<br>(3)Full load continue<br>Ta : 25°C   | VIN: 267VAC<br>VDS:<br>(1). 458.00V<br>(2). 424.00V<br>(3). 430.00V           |
| 6 | PFC Diode            | D1<br>Rated : 600V 4.0A                | I/P : 267VAC<br>I/P : 97VAC<br>O/P : (1)Full Load Turn on<br>(2) Output Short<br>(3)Dynamic Load Full/Min Load 90%Duty/5KHz<br>(4)Dynamic Load Full/Min Load 50%Duty/120Hz<br>Ta : 25°C | 267VAC<br>(1). 444.00V<br>(2). 412.00V<br>(3). 450.00V<br>(4). 452.00V        |
| 8 | Clamp Diode          | D30<br>Rated : 800V 2.0A               | I/P : 267VAC<br>O/P : (1)Dynamic Load Full/Min Load 90%Duty/1KHz<br>(2)Full load continue<br>Ta : 25°C  | (1). 546.00V<br>(2). 546.00V  |

■ SAFETY & E.M.C. TEST

SAFETY TEST

| NO | TEST ITEM            | SPECIFICATION                              | TEST CONDITION   | RESULT   |
|----|----------------------|--|--|--|
| 1  | WITHSTAND VOLTAGE    | I/P-O/P : 4.000KVAC /min<br>2.000KVAC /min | I/P-O/P: 4.400KVAC /min<br>I/P-FG: 2.400KVAC /min<br>Ta : 25°C | I/P-O/P: 1.78mA<br>I/P-FG: 2.28mA<br>NO DAMAGE |
| 2  | ISOLATION RESISTANCE | I/P-O/P : 500VDC>100MΩ                     | I/P-O/P: 500VDC<br>Ta : 25°C/70%RH                             | I/P-O/P: 9999MΩ<br>NO DAMAGE                   |

E.M.C. TEST

| NO | TEST ITEM  | SPECIFICATION                                  | TEST CONDITION  | RESULT                        |
|----|------------|--|---|-------------------------------|
| 1  | HARMONIC   | EN61000-3-2<br>CLASS A                         | I/P : 230VAC /50HZ<br>O/P : FULL LOAD<br>Ta : 25°C            | PASS                          |
| 2  | CONDUCTION | EN55011<br>CLASS B                             | I/P : 230VAC /50HZ<br>O/P : FULL LOAD / 50% LOAD<br>Ta : 25°C | PASS<br>Test by certified Lab |
| 3  | RADIATION  | EN55011<br>CLASS B                             | I/P : 230VAC /50HZ<br>O/P : FULL LOAD<br>Ta : 25°C            | PASS<br>Test by certified Lab |
| 4  | E.S.D      | EN61000-4-2<br>MEDICAL AIR: 8KV / Contact: 6KV | I/P : 230VAC /50HZ<br>O/P : FULL LOAD<br>Ta : 25°C            | CRITERIA A                    |
| 5  | E.F.T      | EN61000-4-4<br>MEDICAL INPUT: 2KV              | I/P : 230VAC /50HZ<br>O/P : FULL LOAD<br>Ta : 25°C            | CRITERIA A                    |
| 6  | SURGE      | IEC61000-4-5<br>MEDICAL L-N:1KV;L/N-PE: 2KV    | I/P : 230VAC /50HZ<br>O/P : FULL LOAD<br>Ta : 25°C            | CRITERIA A                    |



RELIABILITY TEST

| NO | TEST ITEM  | SPECIFICATION   | TEST CONDITION  | RESULT  |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|----|--|---|---|---|-------------------------|---------------------|-------------------------|---|-----|--------|--------|---|-----|--------|--------|---|-----|--------|--------|---|----|--------|--------|---|----|--------|--------|---|-----|--------|--------|---|-----|--------|--------|---|-----|--------|--------|---|---------|--------|--------|----|------|--------|--------|----|----|--------|--------|----|------|--------|--------|----|-------|--------|--------|----|-----|--------|--------|--|
| 1  | TEMPERATURE RISE TEST                                  | MODEL : GSM90A24-P1M<br>1. ROOM AMBIENT BURN-IN : 1.0hrs<br>IP: 230VAC      O/P: 100% LOAD      TA= 20.3°C<br>2. HIGH AMBIENT BURN-IN : 1.0hrs<br>IP: 230VAC      O/P: 100% LOAD      TA= 39.8°C  |   |   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  |   | <table border="1"> <thead> <tr> <th>NO.</th> <th>Position</th> <th>ROOM AMBIENT 20.3°C</th> <th>HIGH AMBIENT Ta: 39.8°C</th> </tr> </thead> <tbody> <tr><td>1</td><td>LF1</td><td>59.1°C</td><td>74.9°C</td></tr> <tr><td>2</td><td>LF2</td><td>76.7°C</td><td>86.6°C</td></tr> <tr><td>3</td><td>BD1</td><td>61.9°C</td><td>78.4°C</td></tr> <tr><td>4</td><td>C5</td><td>68.3°C</td><td>83.8°C</td></tr> <tr><td>5</td><td>L2</td><td>64.4°C</td><td>79.7°C</td></tr> <tr><td>6</td><td>LF3</td><td>65.8°C</td><td>81.5°C</td></tr> <tr><td>7</td><td>Q31</td><td>66.7°C</td><td>83.4°C</td></tr> <tr><td>8</td><td>Q32</td><td>66.7°C</td><td>83.3°C</td></tr> <tr><td>9</td><td>T1 COIL</td><td>75.3°C</td><td>90.8°C</td></tr> <tr><td>10</td><td>Q101</td><td>73.7°C</td><td>90.7°C</td></tr> <tr><td>11</td><td>U2</td><td>68.4°C</td><td>84.7°C</td></tr> <tr><td>12</td><td>C101</td><td>61.5°C</td><td>77.9°C</td></tr> <tr><td>13</td><td>LF101</td><td>54.7°C</td><td>72.0°C</td></tr> <tr><td>14</td><td>C52</td><td>72.1°C</td><td>88.4°C</td></tr> </tbody> </table> | NO.   | Position                | ROOM AMBIENT 20.3°C | HIGH AMBIENT Ta: 39.8°C | 1 | LF1 | 59.1°C | 74.9°C | 2 | LF2 | 76.7°C | 86.6°C | 3 | BD1 | 61.9°C | 78.4°C | 4 | C5 | 68.3°C | 83.8°C | 5 | L2 | 64.4°C | 79.7°C | 6 | LF3 | 65.8°C | 81.5°C | 7 | Q31 | 66.7°C | 83.4°C | 8 | Q32 | 66.7°C | 83.3°C | 9 | T1 COIL | 75.3°C | 90.8°C | 10 | Q101 | 73.7°C | 90.7°C | 11 | U2 | 68.4°C | 84.7°C | 12 | C101 | 61.5°C | 77.9°C | 13 | LF101 | 54.7°C | 72.0°C | 14 | C52 | 72.1°C | 88.4°C |  |
|    |  | NO.   | Position  | ROOM AMBIENT 20.3°C   | HIGH AMBIENT Ta: 39.8°C |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 1   | LF1   | 59.1°C  | 74.9°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 2   | LF2   | 76.7°C  | 86.6°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 3   | BD1   | 61.9°C  | 78.4°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 4   | C5  | 68.3°C  | 83.8°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 5   | L2  | 64.4°C  | 79.7°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 6   | LF3   | 65.8°C  | 81.5°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 7   | Q31   | 66.7°C  | 83.4°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 8   | Q32   | 66.7°C  | 83.3°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 9   | T1 COIL   | 75.3°C  | 90.8°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 10  | Q101  | 73.7°C  | 90.7°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 11  | U2  | 68.4°C  | 84.7°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
|    |  | 12  | C101  | 61.5°C  | 77.9°C                  |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 13 | LF101  | 54.7°C  | 72.0°C  |   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 14 | C52  | 72.1°C  | 88.4°C  |   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 2  | OVER LOAD BURN-IN TEST                                 | NO DAMAGE<br>1 HOUR ( MIN )   | I/P : 230VAC<br>O/P : 128.53% LOAD<br>Ta : 25°C   | TEST : OK   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 3  | LOW TEMPERATURE TURN ON TEST                           | NO DAMAGE<br>1 HOUR ( MIN )   | I/P : 264VAC / 100VAC<br>O/P : FULL LOAD<br>Ta : -30.0°C  | TEST : OK   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 4  | HIGH HUMIDITY<br>HIGH TEMPERATURE<br>HIGH VOLTAGE TEST | AFTER 12 HOURS<br>IN CHAMBER ON<br>CONTROL 40°C<br>NO DAMAGE  | I/P : 272VAC<br>O/P : FULL LOAD<br>Ta : 40°C<br>HUMIDITY= 95.0% RH  | TEST : OK   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 5  | TEMPERATURE COEFFICIENT                                | ±0.03% /(0°C~40°C)  | I/P : 230VAC<br>O/P : FULL LOAD   | ±0.0196% /(0°C~40°C)  |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 6  | STORAGE TEMPERATURE TEST                               | 1. Thermal shock Temperature : -40°C ~ +85°C<br>2. Temperature change rate : 25°C / MIN<br>3. Dwell time low and high temperature : 30 MIN/EACH<br>4. Total test cycle : 5 CYCLE<br>5. Input/Output condition : STATIC  |   | TEST : OK   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 7  | THERMAL SHOCK TEST                                     | 1. Thermal shock Temperature : -35°C ~ +45°C<br>2. Temperature change rate : 25°C / MIN<br>3. Dwell time low and high temperature : 30 MIN/EACH<br>4. Total test cycle : 10 CYCLE<br>5. Input/Output condition :<br>230VAC Full Load AC ON/OFF test turn on 58sec ; turn off 2sec |   | TEST : OK   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 8  | VIBRATION TEST   | 1 Carton & 1 Set<br>(1) Waveform : Sine Wave<br>(2) Frequency : 10~500Hz<br>(4) Acceleration : 2G<br>(5) Test Time : 60 min in each axis (X.Y.Z)<br>(6) Ta : 25°C   |   | TEST : OK   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 9  | CAPACITOR LIFE CYCLE                                   | :SUPPOSE C101 IS THE MOST CRITICAL COMPONENT<br>(1) I/P : 230VAC O/P : FULL LOAD Ta= 25.0°C LIFE TIME<br>(2) I/P : 230VAC O/P : FULL LOAD Ta= 40.0°C LIFE TIME<br>(3) I/P : 230VAC O/P : 75% LOAD Ta= 40.0°C LIFE TIME<br>(4) I/P : 230VAC O/P : 50% LOAD Ta= 40.0°C LIFE TIME    |   | (1). 177817.6 HRS<br>(2). 77916 HRS<br>(3). 152206.9 HRS<br>(4). 270922.4 HRS |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 10 | MTBF   | MIL-HDBK-217F<br>TOTAL FAILURE RATE : 405.6 KHRS  |   |   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |
| 11 | DMTBF /Accelerated Life test                           | Demonstration Mean Time Between Failure (Expected Life): Above 30000HRS @ TA 40°C   |   |   |                         |                     |                         |   |     |        |        |   |     |        |        |   |     |        |        |   |    |        |        |   |    |        |        |   |     |        |        |   |     |        |        |   |     |        |        |   |         |        |        |    |      |        |        |    |    |        |        |    |      |        |        |    |       |        |        |    |     |        |        |  |

|             |        |        |          |
|-------------|--------|--------|----------|
| TEST RESULT | TESTER | REVIEW | APPROVAL |
| PASS        | FRANK  | GESG   | WANGDZ   |

2007/3/20 A50-S014